

Specific Detection of Antibiotics by Silicon On-chip Photonic Crystal Biosensor Arrays

Hai Yan, Chun-Ju Yang, Naimei Tang, Yi Zou, Swapnajit Chakravarty, *Senior Member, IEEE*, Amanda Roth, and Ray T. Chen, *Fellow, IEEE*

Abstract— Photonic crystal (PC) microcavities formed by 2D air holes on silicon-on-insulator substrates were utilized as biosensors to detect antibiotics with high specificity. The antibiotic, gentamicin, with molecular weight of only 478 g/mol, was successfully detected via its binding to corresponding antibody pre-immobilized on the sensor surface. Detection range (in concentration) was extended by combining different types of PC biosensors on a single silicon chip, covering from 0.1nM to 1 μ M. Specificity of detection was also verified on the studied antibiotic.

Index Terms— photonic crystals, silicon photonics, optical biosensors, microcavities, antibiotics

I. INTRODUCTION

THERAPEUTIC drug monitoring helps maximize the therapeutic effect while minimizing adverse effects [1]. Conventional methods have been developed for the measurement of antibiotics, including immunoassays, spectrophotometry, high-performance liquid chromatography (HPLC) and liquid chromatography–mass spectrometry (LC-MS) [2]–[5]. These methods are usually expensive and time-consuming. Innovative detection methods with high sensitivity and low cost are needed. Over the last two decades, on-chip silicon photonic biosensors have become a fast-growing research topic owing to the advantages of high sensitivity, high throughput, and no need for labeling. Various devices, including microring resonators [6]–[9], microdisks [10], silicon nanowires [11], nanoporous silicon waveguides [12], Bragg gratings [13], [14], subwavelength grating waveguides [15], [16], 1D and 2D photonic crystal (PC) microcavities [17]–[22], have been demonstrated. The 2D PC microcavity sensor is unique in its slow light enhanced sensitivity within a miniature footprint and flexibility in

structural design to engineer its sensing properties.

We have previously reported several PC microcavity biosensor structures which consist of a PC microcavity side-coupled to a PC waveguide. The L_n PC microcavity is formed by a row of n missing holes in the Γ -K direction of a hexagonal PC lattice of air holes in silicon (see Fig.1). PC microcavities, such as L13, L21, L55 and L13 with nanoholes, have been reported, offering different minimum detection limits from as low as 1 fM to over 1 μ M for detecting biotin-avidin binding [18], [23]–[25]. In this paper, we report a PC microcavity biosensor array by combining different L-type PC microcavity sensors using a multimode interferometer (MMI) power splitter and demonstrate the detection of antibiotics over a concentration range covering 5 orders of magnitude (from 0.1 nM to 1 μ M). We explored the sensing of gentamicin antibiotics (molecular weight 478 g/mol) by detecting the binding of antibiotics (target) to anti-gentamicin antibody (probe) that was pre-immobilized on the optical sensor surface. The high sensitivity and label-free detection of integrated photonic sensors with PC microcavities makes possible the detection of these small biomolecules. Detection range in concentration was extended by combining different types of PC biosensors on a single silicon sensor chip. Specificity of detection was also verified on the studied antibiotic.

II. DEVICE DESIGN

In a PC microcavity biosensor, the detection limit and sensitivity are determined by factors including quality factor (Q), group index (n_g), fill fraction (f), etc. Increased quality factor results in narrower linewidth of the resonance and enhanced interaction time between the optical mode and the analyte. Therefore, the sensitivity is increased and the detection limit ($D = \lambda/QS$) becomes lower. On the other hand, the slow light effect (high n_g) in the coupling waveguide, which enhances light-matter interaction in the cavity, brings unique advantage for high sensitivity sensing. From L3 to L13 and L55 PC microcavities, with increasing cavity length, the sensors possess improved sensitivity and reduced detection limit owing to increasingly high Q and n_g [18], [23]–[25].

Another critical design consideration is the analyte overlap with cavity modes, characterized by fill fraction (f) [24]:

Manuscript received XX/XX, 2017. This work was supported by Army (USAMRAA) Contract # W81XWH-14-C-0029.

H. Yan, C.-J. Yang, Y. Zou and R. T. Chen are with the Microelectronic Research Center, Department of Electrical and Computer Engineering, The University of Texas at Austin, 10100 Burnet Rd., Austin, TX 78758 USA. (e-mails: hai.yan@utexas.edu, chunjuyang@utexas.edu, yzou@utexas.edu, raychen@uts.cc.utexas.edu)

N. Tang and S. Chakravarty are with Omega Optics Inc., 8500 Shoal Creek Blvd, Austin, TX 78757, USA (e-mails: naimeit@gmail.com, swapnajit.chakravarty@omegaoptics.com).

A. Roth is with Wound Infections Department, Walter Reed Army Institute of Research, Silver Spring, MD 20910, USA (e-mail: amanda.l.roth.mil@mail.mil)

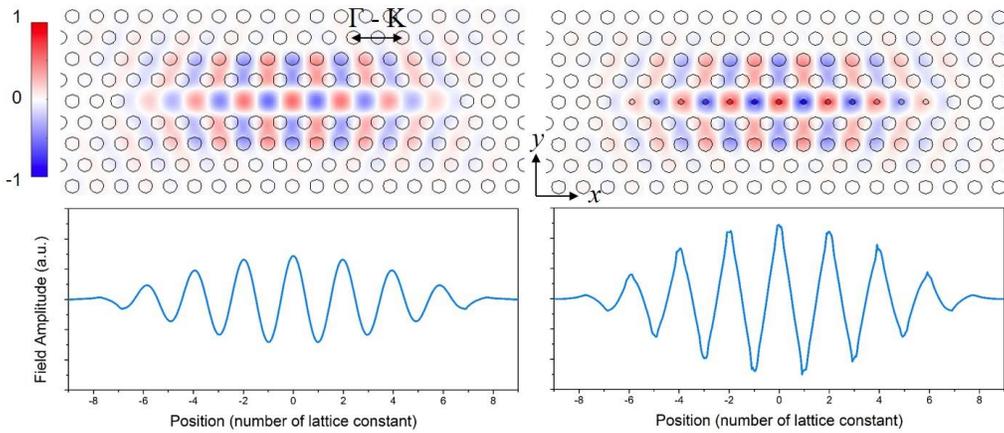


Fig. 1. Mode profiles (E_y) of L13 and L13 with nanoholes PC microcavities.

$$f = \frac{\langle \vec{E}_m | \epsilon | \vec{E}_m \rangle_{V_{liquid}}}{\langle \vec{E}_m | \epsilon | \vec{E}_m \rangle_{V_{liquid+dielectric}}} \quad (1)$$

where \vec{E}_m denotes the electric field of the m th mode and ϵ is the dielectric constant. The sensitivity of the microcavity sensor is proportional to the fill fraction [24]. The L13 with nanoholes microcavity has small holes inside the cavity which results in significantly increased fill fraction ($f=0.14$ for L13 with nanoholes, an increase of 40% from $f=0.10$ for L13 cavity, see Fig. 1). We were able to achieve a high sensitivity (112 nm/RIU) and low detection limit (1 fM) from the L13 with nanoholes biosensors [24].

Considering the above factors that affect the detection range and minimum detection limits of PC biosensors, four distinct types of 2D PC sensors with different geometries were chosen to achieve wide dynamic range detection in the drug molecule sensing. They are L3, L13, L55 and L13 with nanoholes. They were combined in a 1×4 multimode interferometer (MMI) power splitter to allow for simultaneous testing of all microcavities in the same measurement. A schematic of the system is shown in Fig. 2(a). Grating couplers were used to couple continuous wave (CW) light in and out of the waveguide

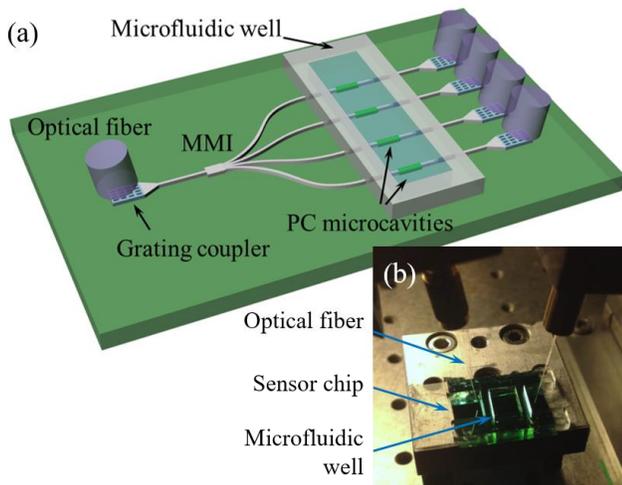


Fig. 2. (a) Schematic of the PC microcavity biosensor array. (b) The sensor chip on a fiber coupling test stage.

devices. Samples containing biomolecules were applied on the PC microcavities inside a microfluidic well made of polydimethylsiloxane (PDMS).

The sensor chip was fabricated on a silicon-on-insulator (SOI) wafer with 250 nm thick silicon device layer. The device pattern was defined by e-beam lithography and transferred to the silicon layer by reactive ion etching. The lattice constant of the PC is designed as $a = 392.5$ nm and the air holes have a radius $r = 108$ nm as in [24]. In L13 PC microcavities with nanoholes device, the nanoholes have a radius of $0.4r = 43$ nm. The grating couplers were designed following the principles in [23] with grating period of 690 nm and duty cycle of 50%. The length and width of the MMI are 123 μm and 16 μm , respectively. All input and output waveguides at the MMI are

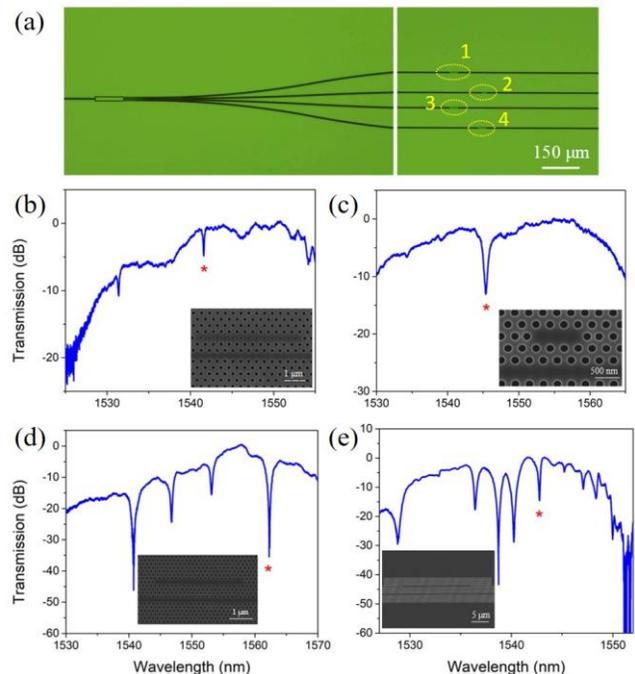


Fig. 3. (a) Stitched microscope image showing the MMI coupler and four PC sensors on the four channels. (b)-(e) Transmission spectra and SEM images of PC microcavities side-coupled to PC waveguides: (b) L13 with nanoholes, (c) L3, (d) L55. Red star markers show the resonance dip used for biosensing test.

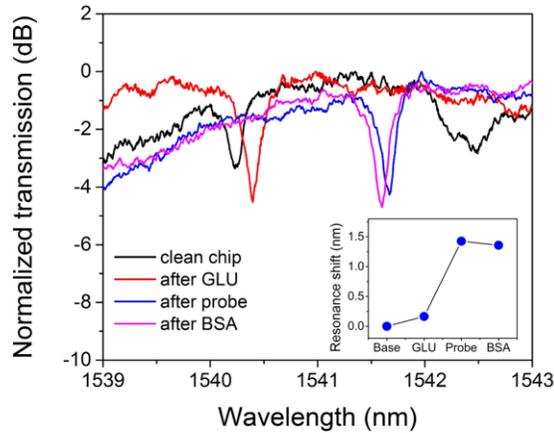


Fig. 4. Transmission spectra of a L13 with nanoholes before and after functionalization. Inset shows the resonance shift at each step. GLU: glutaraldehyde; probe: anti-gentamicin antibody; BSA: bovine serum albumin.

2.5 μ m wide. The output waveguides are separated by 1.5 μ m. Fig. 3(a) shows a stitched microscope image of the MMI and the four PC sensors on the four optical paths. The insets in Fig. 3(b)-(e) show the images of the individual PC sensors observed under scanning electron microscope (SEM).

III. BIOSENSING TEST

The sensor chip needs chemical treatment before the biosensing experiment in order to immobilize probe antibodies covalently. After the sensor chip was fabricated, thermal oxidation is done at 950 $^{\circ}$ C for 5 min to grow about 5 nm silicon dioxide on the sensor surface. The oxide layer serves as the base for subsequent chemical treatment. The chip was next silanized with 2% (v/v) (3-aminopropyl)triethoxysilane (APTES) in toluene. After a thorough clean with toluene, the chip was further treated with 2.5% (v/v) glutaraldehyde in phosphate buffer saline (PBS) to provide an aldehyde group linker that is able to immobilize probe antibodies covalently [26]. After that, a microfluidic well (7mm long \times 5mm wide and 2mm high) made of Polydimethylsiloxane (PDMS) was mounted on the sensor chip (see Fig. 2(b)). The following reaction and test were done in the microfluidic well in a static condition. The probe antibody was immobilized on the sensor surface by dispensing anti-gentamicin antibodies (1mM in PBS) in the microfluidic well and incubating for 60 min after which the device is washed thoroughly with PBS to remove any unbound antibodies. Before target binding test, 1% bovine serum albumin (BSA) was applied to block any binding sites that have not been covered by probe antibodies. After a thorough wash in PBS, the device was ready for antibiotics sensing test.

The transmission spectra of the PC sensors were obtained using a broadband amplified spontaneous emission (ASE) source (1510 nm-1630 nm) and an optical spectrum analyzer (OSA). The measured transmission spectra for the four PC sensors are shown in Fig. 3(b)-(e).

Figure 4 shows the transmission spectra of a L13 with nanoholes PC biosensor before and after the above

functionalization steps. All measurements are done with PBS as background. A red shift of 0.16 nm and 1.43 nm after applying glutaraldehyde and probe (anti-gentamicin antibody) are indications of surface mass accumulation with chemical films (APTES and glutaraldehyde) and immobilized probes. The slight blue shift after applying BSA is probably due to insufficient wash after probe incubation while some probe molecules were washed away at BSA step. After BSA incubation, the chip was washed thoroughly with PBS to create a baseline for target binding test.

All target antibiotics were spiked in 1% BSA in PBS. The sensors were incubated in target solutions for 40 minutes at room temperature and then washed with PBS. Transmission spectra of the PC sensors were measured after each step in the same PBS environment in order to compare the resonance wavelength shifts. The experiments were divided into two parts: (a) sensor array demonstration and (b) specificity verification.

A. Sensor array demonstration

Sensor chips with all four types of PC sensors, L3, L13, L55 and L13 with nanoholes combined by a 1 \times 4 MMI were used. Anti-gentamicin antibody at high concentration of 1mM was used as the probe to create enough binding sites on the sensor surface. Gentamicin concentrations from 1 nM to 10 μ M with a step of an order of magnitude were used as the target to be detected. The resonance shift for each sensor was measured and the corresponding concentration recorded.

B. Specificity verification

In this part, sensor chips with only L13 PC microcavity sensors were used. The chips were activated and immobilized with anti-gentamicin antibody. The chip was then tested with all three antibiotics, all at a concentration of 1 mM. The resonance shift for each antibiotic was recorded.

IV. RESULTS AND DISCUSSION

A wide concentration range (5 orders of magnitude) of gentamicin was measured on a sensor array consisting of four distinct PC sensors (L3, L13, L55 and L13 with nanoholes) following the test procedures in Section III.A to characterize the PC biosensors and the bio-molecular binding. The relative wavelength shift from the baseline for all four devices at different concentrations was extracted from the experimental spectra and plotted in Fig. 5. From this figure, it can be seen that for each type of PC biosensor, there is a linear response region where the resonance shift is almost linearly proportional to the log of the concentration, followed by a saturation region where there is only minimal shift with increased concentration. The data points were fitted with Langmuir equation [17], [27], [28]. From the fitting, the dissociation constant of the binding between gentamicin and anti-gentamicin was calculated. The results are in the range between 0.52 nM and 13 nM. The dose response curves show that L13 with nanoholes sensor produces significantly larger resonance shift and thus has higher sensitivity compared to other PC cavities without nanoholes; among PC cavities without nanoholes, longer cavities show

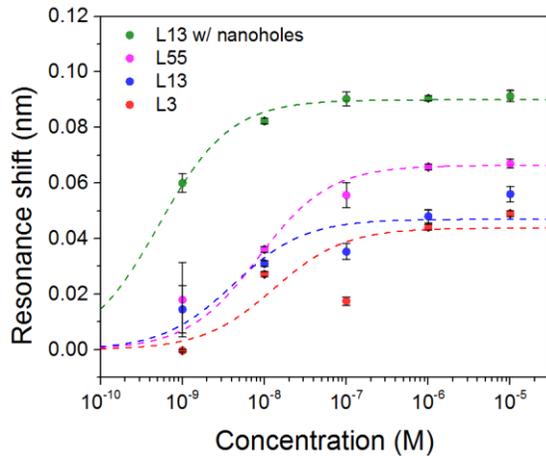


Fig. 5. Resonance shift of the four devices combined in the sensor array when target gentamicin antibiotics were bound to anti-gentamicin antibody on the sensor surface. The colored background and lines indicate the detection range for different PC microcavity biosensors.

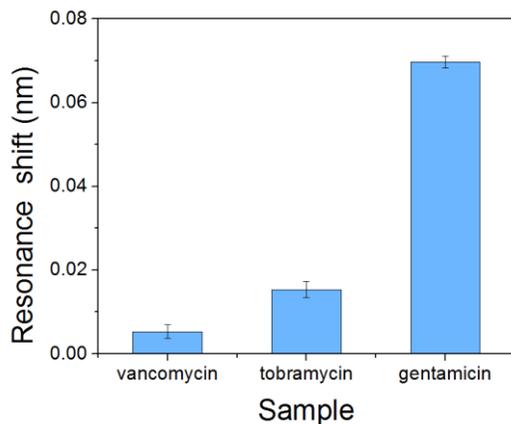


Fig. 6. Resonance shifts in L13 PC microcavity biosensors in the specificity test of gentamicin versus different target antibiotics.

larger shift and higher sensitivity than shorter cavities (from L55, L13 to L3). It can also be seen that L13 with nanoholes sensor begins to saturate at lower target concentration (~ 10 nM) than PC sensors without nanoholes (~ 100 nM to 1μ M). It can be explained by the fact that the optical mode in L13 with nanoholes sensor concentrates in the small-size holes, which reduces the effective sensing region and makes it easier to saturate with biomolecules. With the sensor array containing PC sensors both with and without nanoholes, it is thus possible to cover a wider detection range than using a single type of PC sensor.

The specificity of the PC sensor was verified by measuring responses with antibiotics that do not bind to a specific antibody, as described in Section III.B. Fig. 6 shows the measurement result from the specificity verification test. Anti-gentamicin antibody probe is pre-immobilized on the sensor. The red-shift observed for tobramycin and vancomycin (non-specific bindings) are less than 0.02 nm, even though very high concentrations were introduced (1mM). The shift is much smaller than that from the specific binding of gentamicin (~ 0.07 nm). Thus it shows good specificity in the detection method.

V. CONCLUSION

In summary, PC microcavities formed by 2D air holes on silicon-on-insulator substrates were demonstrated as biosensors to detect specific antibiotics in liquid form. The antibiotic, gentamicin, with molecular weight of only 478 g/mol, was successfully detected via its binding to its corresponding antibody pre-immobilized on the sensor surface. Detection range of concentrations was extended (0.1nM to 1μ M) by combining different types of PC biosensors on a single silicon sensor chip with different minimum sensitivities. Specificity of the detection was also verified.

Our demonstrated silicon photonic biosensing platform can be implemented as a portable lab-on-chip sensing system. By integrating the PC biosensor chip with microfluidics, automated real-time testing can be realized. Furthermore, by utilizing PC filters [19], the device can function as a single-input single-output system, enabling high-throughput sensing tests with largely reduced optical peripheral components.

ACKNOWLEDGEMENT

The authors acknowledge Army (USAMRAA) (Contract # W81XWH-14-C-0029) and AFOSR MURI program (FA9550-08-1-0394) for supporting this research.

REFERENCES

- [1] M. Suryadevara, K. E. Steidl, L. A. Probst, and J. Shaw, "Inappropriate vancomycin therapeutic drug monitoring in hospitalized pediatric patients increases pediatric trauma and hospital costs," *J. Pediatr. Pharmacol. Ther.*, vol. 17, no. 2, pp. 159–65, 2012.
- [2] J. F. Wilson, A. C. Davis, and C. M. Tobin, "Evaluation of commercial assays for vancomycin and aminoglycosides in serum: a comparison of accuracy and precision based on external quality assessment," *J. Antimicrob. Chemother.*, vol. 52, no. 1, pp. 78–82, 2003.
- [3] S. S. Sampath and D. H. Robinson, "Comparison of New and Existing Spectrophotometric Methods for the Analysis of Tobramycin and Other Aminoglycosides," *J. Pharm. Sci.*, vol. 79, no. 5, pp. 428–431, May 1990.
- [4] K. H. Abu-Shandi, "Determination of vancomycin in human plasma using high-performance liquid chromatography with fluorescence detection," *Anal. Bioanal. Chem.*, vol. 395, no. 2, pp. 527–532, 2009.
- [5] C. Cheng *et al.*, "LC-MS/MS method development and validation for the determination of polymyxins and vancomycin in rat plasma," *J. Chromatogr. B*, vol. 878, no. 28, pp. 2831–2838, Oct. 2010.
- [6] M. Iqbal *et al.*, "Label-Free Biosensor Arrays Based on Silicon Ring Resonators and High-Speed Optical Scanning Instrumentation," *IEEE J. Sel. Top. Quantum Electron.*, vol. 16, no. 3, pp. 654–661, 2010.
- [7] M. S. McClellan, L. L. Domier, and R. C. Bailey, "Label-free virus detection using silicon photonic microring resonators," *Biosens. Bioelectron.*, vol. 31, no. 1, pp. 388–392, 2012.
- [8] C.-Y. Chao and L. J. Guo, "Biochemical sensors based on polymer microrings with sharp asymmetrical resonance," *Appl. Phys. Lett.*, vol. 83, no. 8, p. 1527, Aug. 2003.
- [9] A. L. Washburn, L. C. Gunn, and R. C. Bailey, "Label-free quantitation of a cancer biomarker in complex media using silicon photonic microring resonators," *Anal. Chem.*, vol. 81, no. 22, pp. 9499–9506, 2009.
- [10] S. M. Grist *et al.*, "Silicon photonic micro-disk resonators for label-free biosensing," *Opt. Express*, vol. 21, no. 7, p. 7994, Apr. 2013.
- [11] S. Janz *et al.*, "Photonic wire biosensor microarray chip and

- instrumentation with application to serotyping of *Escherichia coli* isolates,” *Opt. Express*, vol. 21, no. 4, pp. 4623–37, 2013.
- [12] X. Wei, J. W. Mares, Y. Gao, D. Li, and S. M. Weiss, “Biomolecule kinetics measurements in flow cell integrated porous silicon waveguides,” *Biomed. Opt. Express*, vol. 3, no. 9, p. 1993, Sep. 2012.
- [13] P. Prabhathan, V. M. Murukeshan, Z. Jing, and P. V. Ramana, “Compact SOI nanowire refractive index sensor using phase shifted Bragg grating,” *Opt. Express*, vol. 17, no. 17, p. 15330, 2009.
- [14] X. Wang *et al.*, “A silicon photonic biosensor using phase-shifted Bragg gratings in slot waveguide,” *J. Biophotonics*, vol. 6, no. 10, pp. 821–828, 2013.
- [15] H. Yan *et al.*, “Unique surface sensing property and enhanced sensitivity in microring resonator biosensors based on subwavelength grating waveguides,” *Opt. Express*, vol. 24, no. 26, p. 29724, Dec. 2016.
- [16] J. Flueckiger *et al.*, “Sub-wavelength grating for enhanced ring resonator biosensor,” *Opt. Express*, vol. 24, no. 14, p. 15672, Jul. 2016.
- [17] F. Liang, N. Clarke, P. Patel, M. Loncar, and Q. Quan, “Scalable photonic crystal chips for high sensitivity protein detection,” *Opt. Express*, vol. 21, no. 26, pp. 32306–12, 2013.
- [18] W.-C. Lai, S. Chakravarty, Y. Zou, Y. Guo, and R. T. Chen, “Slow light enhanced sensitivity of resonance modes in photonic crystal biosensors,” *Appl. Phys. Lett.*, vol. 102, no. 4, p. 41111, Jan. 2013.
- [19] H. Yan *et al.*, “Silicon on-chip bandpass filters for the multiplexing of high sensitivity photonic crystal microcavity biosensors,” *Appl. Phys. Lett.*, vol. 106, no. 12, p. 121103, Mar. 2015.
- [20] A. Di Falco, L. O’Faolain, and T. F. Krauss, “Chemical sensing in slotted photonic crystal heterostructure cavities,” *Appl. Phys. Lett.*, vol. 94, no. 6, pp. 1–4, 2009.
- [21] S. Mandal, J. M. Goddard, and D. Erickson, “A multiplexed optofluidic biomolecular sensor for low mass detection,” *Lab Chip*, vol. 9, no. 20, p. 2924, 2009.
- [22] S. Pal, E. Guillermain, R. Sriram, B. L. Miller, and P. M. Fauchet, “Silicon photonic crystal nanocavity-coupled waveguides for error-corrected optical biosensing,” *Biosens. Bioelectron.*, vol. 26, no. 10, pp. 4024–4031, Jun. 2011.
- [23] Yi Zou *et al.*, “Cavity-Waveguide Coupling Engineered High Sensitivity Silicon Photonic Crystal Microcavity Biosensors With High Yield,” *IEEE J. Sel. Top. Quantum Electron.*, vol. 20, no. 4, pp. 171–180, Jul. 2014.
- [24] S. Chakravarty, A. Hosseini, X. Xu, L. Zhu, Y. Zou, and R. T. Chen, “Analysis of ultra-high sensitivity configuration in chip-integrated photonic crystal microcavity bio-sensors,” *Appl. Phys. Lett.*, vol. 104, no. 19, p. 191109, 2014.
- [25] W.-C. Lai, S. Chakravarty, Y. Zou, and R. T. Chen, “Silicon nano-membrane based photonic crystal microcavities for high sensitivity bio-sensing,” *Opt. Lett.*, vol. 37, no. 7, p. 1208, Apr. 2012.
- [26] A. Subramanian, S. J. Kennel, P. I. Oden, K. B. Jacobson, J. Woodward, and M. J. Doktycz, “Comparison of techniques for enzyme immobilization on silicon supports,” *Enzyme Microb. Technol.*, vol. 24, no. 1–2, pp. 26–34, Jan. 1999.
- [27] I. Langmuir, “The adsorption of gases on plane surfaces of glass, mica and platinum,” *J. Am. Chem. Soc.*, vol. 40, no. 9, pp. 1361–1403, Sep. 1918.
- [28] S. Zlatanovic *et al.*, “Photonic crystal microcavity sensor for ultracompact monitoring of reaction kinetics and protein concentration,” *Sensors Actuators, B Chem.*, vol. 141, no. 1, pp. 13–19, 2009.

Hai Yan received his B.S. degree in optical information science and technology from Huazhong University of Science and Technology, Wuhan, China, in 2010 and M.S. degree in electronic engineering from Tsinghua University, Beijing, China, in 2013. He is currently working towards his Ph.D. degree at the University of Texas at Austin, TX, USA. His research interests include silicon photonics, nonlinear optics, integrated photonic biosensors, silicon-organic hybrid nanophotonic devices.

Chun-Ju Yang is currently a Ph.D. student at the University of Texas at Austin, TX, USA. Her research interests include graphene modulators, metamaterials biosensing, plasmonics, nano-photonics, integrated photonic biosensors.

Naimei Tang received her B.S. in Chemistry from Jilin University in 1984 and her Ph.D. in Biochemistry from Dalian Medical University, Dalian, China in 1996. Since then, she has held several position, including Research Associate in Dept. of Surgery at VA hospital, Dept. of Internal Medicine, Dept. of Rheumatology, at Wayne State University, Detroit, MI. From 2006-2012, Dr. Tang was Assistant Professor in Division of Rheumatology and Internal Medicine at Wayne State University, Detroit, MI. Since 2009, Dr. Tang has served as Clinical Trial Investigator/Assistant Professor at the National Cancer Center National Center of Vermiculite and Asbestos related Cancer (NCVAC), Karmanos Cancer Institute, Wayne State University, Detroit, MI. She has over 30 publications in peer-reviewed journals and conference proceedings. At Wayne State University. Dr. Tang was the PI and co-PI in several grants from NIH and EPA for the development of biomarkers for breast cancer and mesothelioma respectively.

Yi Zou received his Ph.D. degree in Electrical and Computer Engineering in 2014 from the University of Texas at Austin, Austin. Currently he is an assistant professor in School of Information Science and Technology in ShanghaiTech University, Shanghai. His research interests include integrated photonics, nanophotonics and fiber optics.

Swapnajit Chakravarty received his PhD in Electrical Engineering from the University of Michigan, Ann Arbor, MI in 2007, Masters in Electrical Engineering from the University of Cincinnati, Cincinnati, OH in 2003 and Bachelors in Electrical Engineering from Jadavpur University, Kolkata, India in 2001. He has been an active researcher in photonic crystal (PC) devices in the past 13 years. His research area includes electrically and optically injected 2D PC lasers and light emitting arrays and PC sensors. His recent research interest is to utilize PC slot waveguide devices and PC microcavity devices for optical sensing and spectroscopy. He is proficient with optical device design and fabrication, and has solid foundation in semiconductors, integrated optics and PC devices for sensing and spectroscopy. Dr. Chakravarty has over 100 publications in refereed journals and conferences. His research on electrically injected 2D quantum dot PC light emitting arrays received critical acclaim with the Raith Micrograph Award in 2006. In 2013, Dr. Chakravarty was promoted to Senior Member in SPIE and IEEE.

Amanda Roth received her PhD from Creighton University in Medical Microbiology and Immunology. She currently services in the United States Army as a Research Microbiologist in the Bacterial Diseases Branch of the WRAIR. Her professional interests include infectious disease diagnostics, carbapenem-resistant bacteria, and scientific communications. She is also a Board-certified Medical Laboratory Scientist and certified Science and Technology Manager.

Ray T. Chen (M'91–SM'98–F'04) received the B.S. degree in physics from the National Tsing Hua University, Hsinchu City, Taiwan, in 1980, the M.S. degree in physics in 1983, and the Ph.D. degree in electrical engineering in 1988, both from the University of California. He is the Keys and Joan Curry/Cullen Trust Endowed Chair at The University of Texas Austin. Chen is the director of the Nanophotonics and Optical Interconnects Research Lab, at the Microelectronics Research Center. He is also the director of two MURI-Centers: 1. Silicon Nanomembranes and 2. Energy-efficient Optical Interconnects and Computing. His research topics are focused on three main subjects: (1) Nano-photonic passive and active devices for sensing and interconnect applications, (2) Thin film guided-wave optical interconnection and packaging for 2D and 3D laser beam routing and steering, and (3) True time delay (TTD) wide band phased array antenna (PAA). His group at UT Austin has reported its research findings in more than 820 published papers, including over 100 invited papers. He holds over 35 patents. He has chaired or been a program-committee member for more than 110 domestic and international conferences organized by IEEE, SPIE, OSA, and PSC. He has served as an editor, co-editor or coauthor for over twenty books. He has also served as a consultant for various federal agencies and private companies and delivered numerous invited talks to professional societies. He is a Fellow of IEEE, OSA, and SPIE.